



Technical data sheet TDS0065

DUAL PREMIER INFRARED SENSOR FOR HYDROCARBONS and CARBON DIOXIDE Certified versions types MSH-DP-HC/CO2 and MSHia-DP-HC/CO2



Great Britain
Europe
France
Germany
Italy
Switzerland
USA

Patent Numbers

GB 2 401 432 & GB 2 403 291
EP 1544603 & EP 1818667-Pending
EP [FR] 1544603
EP [DE] 1544603
EP [I] 1544603
EP [CH] 1544603
7, 244, 939

Other World Patents Pending

FEATURES

- ★ Combines all the features of the hydrocarbon and carbon dioxide Premier sensors, enabling the measurement of two different gases with one sensor.
- ★ No increase in physical size or power consumption when compared with a single gas Premier sensor. Ideal for portable, battery powered instruments.
- ★ Contains all the necessary optics, electronics and firmware to provide TWO linearised, temperature-compensated outputs.
- ★ Digital output for direct interface to host circuitry.
- ★ The hydrocarbon channel can be used to measure methane from 0 to 100% volume with an auto-ranging feature that provides the optimum resolution in both the % LEL range and the % volume range. Has equal performance to a 0-5% volume methane sensor AND a 0-100% volume methane sensor.
- ★ The hydrocarbon channel can be configured for any of the hydrocarbon gases available in the single-gas Premier range.
- ★ All sensor types are user configurable using configuration equipment available from Dynamant.
- ★ Fast track route for original equipment manufacturers to introduce the latest infrared technology – without any specialist knowledge.
- ★ Internal Flash memory allowing sensor firmware updates via configuration equipment.



Dynamant Limited

Premier House · The Village · South Normanton · Derbyshire · DE55 2DS · UK.

Tel: 44 (0)1773 864580 · Fax: 44 (0)1773 864599

email: sales@dynamant.com · www.dynamant.com

CERTIFICATION DETAILS

European ATEX Certification	Sensor type MSH-P	Sensor type MSHia-P
Approval body	SIRA	
Certificate Number	SIRA 04ATEX1357U	
Test Standards	EN60079-0:2006, EN60079-1:2004, EN60079-11:2007, EN60079-26:2006	
Certification Codes	I M2 Ex d I & II 2 G Ex d IIC	I M1 Ex d+ia I Ma & II 2 G Ex d IIC Gb
Input parameters	0.8W max, 30V max.	Ui=6V dc, Pi=0.8W
Operating temperature	-20°C to +60°C	
International IECEx Certification	Sensor type MSH-P	Sensor type MSHia-P
Approval body	SIRA	
Certificate Number	IECEX SIR 05.0053U	
Test Standards	IEC 60079-0:2004, IEC60079-1:2003, EN60079-26:2006	
Certification Codes	Ex d I & Ex d IIC	Ma Ex d+ia I & Gb Ex d IIC
Input parameters	0.8W max, 30V max.	Ui=6V dc, Pi=0.8W
Operating temperature	-20°C to +60°C	
North American Certification	Sensor type MSH-P	
Approval body	Underwriters Laboratory Inc.	
File Reference	E229543	
Test Standards	UL913 Fifth Edition	
Hazardous Locations	Class 1 Groups A, B, C and D, T4 with 60°C ambient	
Input parameters are defined for certification purposes only, refer to the "Specification" table on page 7 for the sensor operating voltage and temperature range.		

DESCRIPTION

Dynamant infrared sensors operate by using the NDIR principle to monitor the presence of target gas. The sensor contains a long life tungsten filament infrared light source, an optical cavity into which gas diffuses, temperature compensated pyroelectric infrared detectors, an integral semiconductor temperature sensor and electronics to process the signals from the pyroelectric detector .


The sensor uses a digital output for direct communications with instrument electronics. The digital output is a UART format comprising 8 data bits, 1 stop bit and no parity. Refer to specification for available baud rates.


Hydrocarbon Response Characteristics

The Premier range of hydrocarbon infrared gas sensors are calibrated to provide an output signal linearised for a specific gas type and concentration during manufacture.

However, the sensor will also respond to a range of other hydrocarbon gases. The following graphs show the relative response of a methane sensor, and a propane sensor, to some of the common hydrocarbons.

These characteristics can be used as a guide to setting up the associated instrument alarm levels.






Note – Refer to data sheet TDS0050 for additional cross reference data

Hydrocarbon Temperature Compensation

The Premier sensor is temperature compensated over the range of -20°C to +50°C. The output variation is $\pm 2\%$ FSD or $\pm 10\%$ of the reading up to 50% FSD and $\pm 15\%$ of the reading from 50% to 100% FSD, which ever is greater.


The following graph is based on the hydrocarbon sensor being characterised for methane.



Hydrocarbon Linearity


The Premier sensor linearity at ambient temperature is $\pm 2\%$ FSD or $\pm 10\%$ of the reading which ever is greater.

The following graph is based on the hydrocarbon sensor being characterised for methane, data based on 24 sensors.



Carbon dioxide Temperature Compensation


The Premier sensor is temperature compensated over the range of -20°C to $+50^{\circ}\text{C}$. The output variation is $\pm 0.1\%$ v/v or $\pm 10\%$ of the reading up to 50% FSD and $\pm 15\%$ of the reading from 50% to 100% FSD, which ever is greater.



Carbon dioxide Linearity

The Premier sensor linearity at ambient temperature is $\pm 2\%$ FSD or $\pm 10\%$ of the reading which ever is greater.

The following graph is based on the 0-5% v/v sensor, data for 24 sensors.



Calibration options

Dynamant recommend a maximum interval of 12 months between calibration checks. A small amount of zero drift can be accommodated by re-zeroing the gas detector against the sensor. The degree of drift that is acceptable should be determined by the user. Note that the subsequent change in gas reading will be greater than the change in zero reading. If the sensor requires either a "Zero" or "Span" adjustment, there are three methods that can be used:

- 1) By using the "Premier Configuration Unit"
When used in conjunction with dedicated PC software, this device uses the data communication pins on the sensor to provide a means of calibration. Refer to data sheet TDS0043 for additional information.
- 2) By using the data communications pins and software written in accordance with the protocol supplied by Dynamant.
- 3) By using the "Manual Calibration" feature available with firmware version 1.5.2R.
"Zero" and "Span" operations can be performed by momentarily connecting the data communication pins to the negative supply pin. Refer to data sheet TDS0064 for full instructions. The "Manual Calibration" option must be specified when the sensors are ordered.

Sensor warm-up time

When power is first applied to the sensor, the voltage at the output pin is held at a pre-determined level. The default setting for this start-up value is the "zero gas" value. This condition is maintained for a default "warm-up" time of 15 seconds, after this time the output voltage represents the calculated gas value. Sensors can take up to 1 minute to indicate the correct gas reading.

Note: the sensor can calculate any reading from -100% FSD to +200% FSD in the first minute.

The output value that is read using the communications pins is always held at zero during the “warm-up” time.

The duration of the “warm-up” time can be pre-programmed to alternative values at the time of ordering sensors.

Temperature transients and gas flow rates.

The Premier sensor employs a pyroelectric detector, the output from which can be disrupted by sudden changes in temperature. If there is an excessive change in the ambient temperature, gas sample temperature or flow rate, then the output signal will be momentarily frozen. Correct operation is restored when the effects of the transient have settled. Rates of change in the ambient temperature should be restricted to 2°C/minute and gas flow rates kept below 600 cc/minute.

Power supply considerations

The sensor power supply rise time must be less than 50 mS to ensure correct operation. Operation outside the range of 3 – 5 V dc will result in either fault indication, or the sensor will not function correctly.

Sensor over-range condition

The sensor will continue to provide a reading up to 200% of the full scale value; at this point the reading is clamped, regardless of any further increase in detected gas level. The linearity of the reading is only guaranteed up to the full scale for the sensor; the over-range condition should therefore be determined and indicated by the host instrument.

Sensor fault indication

The sensor constantly performs checks on the internal memory contents, the incoming supply voltage and the analogue signal values. These checks are used to ensure that the sensor is operating within its correct parameters, and that no internal faults have developed.

If a fault condition is detected, the output reading is set to the -100% full scale value.

Digital interface

The digital communication pins “RX” and “TX” operate at a 2.8V logic level. When interfacing to external circuitry that uses a higher voltage level it is necessary to limit the current that can flow. The external voltage level should be 5V maximum and a 3K3 resistor should be used in series with each communication pin.

Warranty information

All Dynamant Premier sensors carry a two year warranty against defects in materials and workmanship. The warranty is invalidated if the sensors are used under conditions other than those specified in this data sheet.

Particular attention should be paid to the following criteria:

- **Observe the correct supply polarity**
- **Do not exceed the maximum rated supply voltage of 5V**
- **Do not solder directly to the sensor pins**
- **Do not expose the sensor to corrosive gases**
- **Do not allow condensation to take place within the sensor**

GENERAL SPECIFICATION

Operating Voltage Range:	3.0 – 5.0 V d.c.
Operating Current:	Constant current operation, current range 75 – 85mA
Operating temperature range:	-20°C to +50°C (-4°F to 122°F)
Warm up time:	To final zero \pm 2% of full scale: 1 minute @ 20°C (68°F) ambient
Storage temperature range:	-20°C to +50°C (-4°F to 122°F)
Humidity range:	0 to 95% RH non-condensing.
Digital signal format:	8 data bits, 1 stop bit, no parity. 2.8V logic level
Standard baud rates:	38,400, 19,200, 9600
User configurable parameters:	Full-scale value, resolution, Sensor 'zero' function Sensor 'span' function
MTBF:	> 5 years
Weight :	15 grams

HYDROCARBON CHANNEL SPECIFICATION


Methane measuring range:	0 – 100% volume
Hydrocarbon measuring range	0 – 100% LEL equivalent
Resolution: (Methane calibration)	0.01% vol. methane for readings up to 10% methane, 0.1% vol. methane for readings from 10% vol. up to 100% vol.
Accuracy:	\pm 2% of full scale @ 20°C (68°F), 1 bar pressure, applied gas 2.5% volume methane.
Response Time T₉₀:	<30s @ 20°C (68°F) ambient
Zero Repeatability:	\pm 1% of full scale @ 20°C (68°F) ambient
Span Repeatability:	\pm 2% of full scale @ 20°C (68°F) ambient
Long term zero drift:	\pm 1% of full scale per month @20°C (68°F) ambient, (max \pm 3% of full scale per year)
Temperature performance: <small>* May not be applicable when using gas cross-reference factors</small>	\pm 10% of reading up to 50% of full scale, \pm 15% of reading from 50% to 100% of full scale, or 2% of full scale whichever is greater over the range -20°C to +50°C (-4°F to 122°F)

CARBON DIOXIDE CHANNEL SPECIFICATION

Measuring ranges:	0 - 5%, 0-4%, 0-3%, 0-2%, 0-1% volume CO ₂
Resolution:	0.01% volume CO ₂ .
Accuracy:	\pm 2% of full scale @ 20°C (68°F), 1 bar pressure, applied gas 2.5% volume CO ₂ .
Response Time T₉₀:	<30s @ 20°C (68°F) ambient
Zero Repeatability:	\pm 500ppm @ 20°C (68°F) ambient
Span Repeatability:	\pm 500ppm @ 20°C (68°F) ambient
Long term zero drift:	\pm 500ppm / month @ 20°C (68°F) ambient
Operating temperature range:	-20°C to +50°C (-4°F to 122°F)
Temperature performance:	\pm 10% of reading up to 50% of full scale and \pm 15% of reading from 50% to 100% of full scale over the range -20°C to +50°C (-4°F to 122°F)

MECHANICAL DETAIL

NOTES

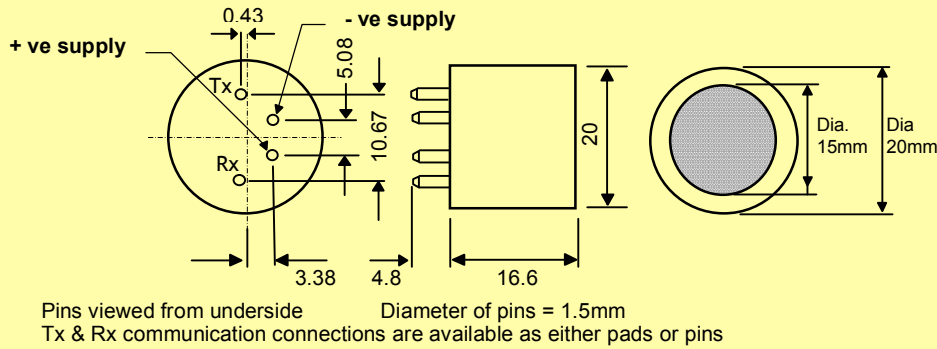

1. DIMENSIONS WITHOUT TOLERANCES ARE NOMINAL.
2. RECOMMENDED PCB SOCKET WEARNES CAMBION LTD CODE: 450-3326-01-06-00.
3. WEIGHT: 15g
4. USE ANTI-STATIC PRECAUTIONS WHEN HANDLING
5. DO NOT CUT PINS
6. DO NOT SOLDER DIRECTLY TO PINS

NOTE – The above pin configuration is shown for the POSITIVE version of the sensor. The NEGATIVE version has the +ve and –ve supply pin positions exchanged. See ordering details.

Ordering Details

In order to completely specify the type of sensor that is required, the customer needs to provide the following information:-


- An Order Code (see below) that specifies the sensors' basic physical and electrical characteristics.
- The sensor configuration requirements.

EXAMPLE OF ORDER CODES

Available sensor options:

F = Replaceable, self adhesive microporous PTFE filter

MSH – DP / HC / CO2 / P / F



Option
FILTER : BLANK = OMITTED
F = FITTED

SUPPLY POLARITY : P = Positive
N = Negative

GAS TYPES : HC = Hydrocarbon
CO2 = Carbon dioxide

DUAL PREMIER SENSOR

TYPE MSH or MSHia (For Mining M1 applications only)

CONFIGURATION OPTIONS

(To be stated on customer order in addition to the Order Code)

1. Communication speed – 38,400 baud (default), specify alternative rate if required.

Dynamant reserve the right to alter technical specifications without prior notice